

1. INTENDED USE

Truenat[®] Malaria Pf (REF 601020005 / 601020020 / 601020025 / 601020050 / 601020100 / 601020200) is a chip-based Real Time Polymerase Chain Reaction (PCR) test for the quantitative detection of *Plasmodium falciparum* in human blood specimen and aids in the differential diagnosis of infection with Malaria caused by *Plasmodium falciparum* (Pf). **Truenat[®] Malaria Pf** runs on **Truelab[®] Real Time micro PCR Analyzers**.

2. INTRODUCTION

Falciparum malaria is a life threatening disease caused by the protozoan parasite, *Plasmodium falciparum*, which is transmitted via the bite of an infected female *Anopheles* mosquito. In the human body, the parasites multiply in the liver and then infect red blood cells. *Plasmodium falciparum* is known to cause the most dangerous malignant malaria which has the highest rate of complications and mortality. Early and accurate diagnosis of Falciparum malaria is necessary to initiate appropriate treatment, check transmission of the disease and prevent death. Microscopic examination of stained blood smears is still considered as the "gold standard" for detection of malaria parasitemia. However in comparison to PCR methods, these are reported to be only 80-90% sensitive. Nested PCR and real time PCR present higher sensitivity and specificity to malaria diagnosis compared to light microscopy. However PCR or Real Time PCR tests have so far been restricted to centralized reference laboratories as they require skilled manpower and elaborate infrastructure. Also the turnaround time for results could take a few days.

The **Truelab[®] Real Time micro PCR System** enables decentralization and near patient diagnosis of *P. falciparum* malaria by making real time PCR technology rapid, simple, robust and user friendly and offering "sample to result" capability even at resource limited settings. This is achieved through a combination of lightweight, portable, mains / battery operated **Truelab[®] Real Time micro PCR Analyzer** and **Trueprep[®] AUTO/AUTO v2 Universal Cartridge Based Sample Prep Device** and room temperature stable **Truenat[®] micro PCR chips** and **Trueprep[®] AUTO/AUTO v2 Sample Prep kits** so that even the peripheral laboratories with minimal infrastructure and minimally trained technician can easily perform these tests routinely in their facilities and report PCR results in less than an hour. Moreover, with these devices PCR testing can also be initiated in the field level, on site.

Truenat[®] Malaria Pf is a disposable, room temperature stable, chip-based Real Time PCR test with dried MgCl₂ in reaction well and freeze dried PCR reagents in microtube performing Real Time PCR test for detection and diagnosis of *Plasmodium falciparum* and runs on the **Truelab[®] Real Time micro PCR Analyzer**. It requires only six (6) µL of purified DNA to be added to the reaction well for the analysis. The intelligent chip also carries test and batch related information including standard values for quantitation. The **Truenat[®] Malaria Pf** chip also stores information of used test to prevent any accidental re-use of the test.

NOTE :Truelab[®] / Truenat[®] / Trueprep[®] / Truepet[®] are all trademarks of Molbio Diagnostics Private Limited.

The **Truelab[®] Real Time micro PCR Analyzer** is protected by the following patents and patents granted: IN 2313/CHE/2007 (Patent No. 281573), WO2009/047804 and corresponding claims of any foreign counterpart(s) thereof.

The **Truenat[®] micro PCR chip** is protected by the following patents and patents pending: IN 2312/CHE/2007, WO 2009/047805 and corresponding claims of any foreign counterpart(s) thereof.

3. PRINCIPLE OF THE TEST

Truenat[®] Malaria Pf works on the principle of Real Time Polymerase Chain Reaction based on Taqman chemistry. The DNA from the patient blood sample is first extracted using **Trueprep[®] AUTO/AUTO v2 Universal Cartridge Based Sample Prep Device** and **Trueprep[®] AUTO/AUTO v2 Universal Cartridge Based Sample Prep kit**. The **Truenat[®] Malaria Pf** chip is placed on the chip tray of the **Truelab[®] Real Time micro PCR Analyzer**. Six (6) µL of the purified DNA is then dispensed using the provided micropipette and tip into the microtube containing freeze dried PCR reagents and allowed to stand for 30-60 seconds to get a clear solution. **△ No mixing by tapping, shaking or by reverse pipetting should be done.** Six (6) µL of this clear solution is then pipetted out using the same pipette and tip and dispensed into the reaction well of the **Truenat[®] Malaria Pf** chip and the test is started. A positive amplification causes the dual labeled fluorescent probe in the **Truenat[®] Malaria Pf** chip-based Real Time PCR test to release the fluorophores in an exponential manner which is then captured by the built-in opto-electronic sensor and displayed as amplification curve on the analyzer screen, on a real time basis during the test run. The Cycle threshold (Ct) is defined as the number of amplification cycles required for the fluorescent signal to cross the threshold (i.e. exceed the background signal). Ct levels are inversely

proportional to the amount of target nucleic acid in the sample. (i.e. the lower the Ct level the greater is the amount of target nucleic acid in the sample). Ct value is linearly correlated with the amount of target DNA present in the sample, enabling quantitative estimation of the analyte. Standard values for every batch are present in the **Truenat[®] Malaria Pf** chip and the analyzer automatically compares these with the Ct values of the test sample to provide a quantitative result. In the case of negative samples, amplification does not occur and a horizontal amplification curve is displayed on the screen during the test run. At the end of the test run, Falciparum "DETECTED" or "NOT DETECTED" result is displayed and in positive cases, Ct values and parasites per microlitre (P/µL) is also displayed on the screen. Based on the detection of the Internal Positive Control (IPC), the validity of the test run is also displayed. The IPC is a full process control that undergoes all the processes the specimen undergoes - from extraction to amplification thereby validating the test run from sample to result. Absence of or shift of IPC Ct beyond a pre-set range in case of negative samples invalidates the test run. While IPC will co-amplify in most positive cases also, in some specimen having a high target load, the IPC may not amplify, however the test run is still considered valid. The results can be printed via Bluetooth using the **Truelab[®] micro PCR printer** or transferred to the lab computer/or any remote computer via Wifi or 3G/ GPRS network. Upto 20000 results in **Truelab[®] Uno Dx/ Duo/Quattro** can be stored on the analyzer for future recall and reference.

4. TARGET SELECTION

The target sequence for this kit has been taken from the erythrocyte binding protein (EBP) gene which is expressed on the surface of the merozoites. EBP is involved in the parasite's invasion of the red blood cells (RBC) by pathways that are specific to *Plasmodium falciparum*. The region selected is specific for *P. falciparum*.

5. CONTENTS OF THE Truenat[®] Malaria Pf KIT

- A. Individually sealed pouches, each containing
1. **Truenat[®] Malaria Pf** micro PCR chip.
 2. Microtube with freeze dried PCR reagents.
 3. DNase & RNase free pipette tip.
 4. Desiccant pouch.
- B. Package Insert.

REF	601020005	601020020	601020025	601020050	601020100	601020200
▽	5T	20T	25T	50T	100T	200T

6. CONTENTS OF THE Trueprep[®] AUTO Universal Sample Pre-treatment Pack

- A. Lysis Buffer.
B. Disposable transfer pipette (graduated).
C. Package Insert.

REF	60205AB05	60205AB20	60205AB25	60205AB50	60205AB100	60205AB200
▽	5T	20T	25T	50T	100T	200T

7. STORAGE AND STABILITY

Truenat[®] Malaria Pf is stable for two (2) years from the date of manufacture if stored between 2-30°C. It is also stable for upto one (1) month at temperatures up to 45°C. Avoid exposure to light or elevated temperatures (above recommended levels). Do not freeze.

Trueprep[®] AUTO Universal Sample Pre-treatment Pack is stable for two (2) years from the date of manufacture if stored between 2-40°C. It is also stable for one (1) month at temperatures upto 45°C. Do not freeze.

8. MATERIALS REQUIRED BUT NOT PROVIDED WITH THE KIT

Truelab[®] Real Time micro PCR Workstation (REF 623010001 / 633010001 / 643010001 / 653010001) consisting of

1. **Trueprep[®] AUTO/AUTO v2 Universal Cartridge Based Sample Prep Device** (REF 603041001 / 603042001).
2. **Truelab[®] Uno Dx / Truelab[®] Duo / Truelab[®] Quattro Real Time micro PCR Analyzer** (REF 603021001 / 603022001 / 603023001).
3. **Truelab[®] micro PCR Printer** (REF 603050001).
4. **Truepet[®] SPA fixed volume precision micropipette - 6 µl** (REF 604070006).
5. **Truelab[®] Microtube Stand** (REF 603070001).

Also required additionally are: **Trueprep[®] AUTO Universal Sample Pre-treatment Pack** (REF60205AB05 / REF60205AB20 / REF60205AB25 / REF60205AB50 / REF60205AB100 / REF60205AB200), **Trueprep[®] AUTO Universal Cartridge Based Sample Prep Kit** (REF60203AR05 / REF60203AR25 / REF60203AR50 / REF60203AR100) or **Trueprep[®] AUTO v2 Universal Cartridge Based Sample Prep Kit** (REF60207AR05 / REF60207AR25 / REF60207AR50 / REF60207AR100), **Truenat[®] Positive Control Kit - Panel IV** (REF 801040008), Powder free disposable gloves, waste disposal container with lid.

9. SPECIMEN PREPARATION FOR EXTRACTION WITH Trueprep[®] AUTO/AUTO v2

Truenat[®] Malaria Pf requires purified nucleic acids from blood specimen that are extracted using the **Trueprep[®] AUTO/AUTO v2 Universal Cartridge based Sample Prep Device** and **Trueprep[®] AUTO/AUTO v2 Universal Cartridge based Sample Prep kit**. Sample must be pre-treated using **Trueprep[®] AUTO Universal Sample Pre-treatment pack**. Transfer 250µl of blood specimen using the transfer pipette provided

into the Lysis buffer tube provided and mix well. (Refer to the package insert of **Trueprep® AUTO** Universal Sample Pre-treatment Pack for further details).

Sample Storage and Transportation:

Sample Pre-treatment decontaminates the specimen and makes it ready for storage / transportation / extraction. The specimen in this form is stable for up to 3 days at 40°C and 1 week at 30°C.

Nucleic acid extraction: Use the entire content of lysis buffer tube containing Specimen for further procedure with the **Trueprep® AUTO/AUTO v2** Universal Cartridge Based Sample Prep Device and **Trueprep® AUTO/AUTO v2** Universal Cartridge Based Sample Prep Kit (Refer to the User Manual of **Trueprep® AUTO/AUTO v2** Universal Cartridge Based Sample Prep device and the package insert of **Trueprep® AUTO/AUTO v2** Universal Cartridge Based Sample Prep kit for details). **△** Dispose off the lysis buffer tube and transfer pipette after use, as per the section on "Disposal and Destruction" (Section 17).

10. SAFETY PRECAUTIONS

1. For *in vitro* diagnostic use only.
2. Bring all reagents and specimen to room temperature (20 - 30°C) before use.
3. Do not use kit beyond expiry date.
4. Carefully read the User Manuals, package inserts and Material Safety Data Sheets (MSDS) of all the components of the **Truelab® Real Time micro PCR System** before use.
5. All materials of human origin should be handled as though potentially infectious.
6. Do not pipette any material by mouth.
7. Do not eat, drink, smoke, apply cosmetics or handle contact lenses in the area where testing is done.
8. Use protective clothing and wear disposable gloves when handling samples and while performing sample extraction.

11. PROCEDURAL PRECAUTIONS

1. Check all packages before using the kit. Damage to the packaging does not prevent the contents of the kit from being used. However, if the outer packaging is damaged the user must confirm that individual components of the kit are intact before using them.
2. Do not perform the test in the presence of reactive vapours (e.g. from sodium hypochlorite, acids, alkalis or aldehydes) or dust.
3. While retrieving the **Truenat® Malaria Pf** micro PCR chip, microtube and the DNase & RNase free pipette tip from the pouch, ensure that neither bare hands nor gloves that have been used for previous tests are used.

12. PROCEDURAL LIMITATIONS

1. Optimal performance of this test requires appropriate specimen collection, handling, storage and transport to the test site.
2. Though very rare, mutations within the highly conserved regions of the target genome where the **Truenat®** assay primers and/or probe bind may result in the under-quantitation of or a failure to detect the presence of the concerned pathogen.
3. The instruments and assay procedures are designed to minimize the risk of contamination by PCR amplification products. However, it is essential to follow good laboratory practices and ensure careful adherence to the procedures specified in this package insert for avoiding nucleic acid contamination from previous amplifications, positive controls or specimens.
4. A specimen for which the **Truenat®** assay reports "Not Detected" cannot be concluded to be negative for the concerned pathogen. As with any diagnostic test, results from the **Truenat®** assay should be interpreted in the context of other clinical and laboratory findings.

13. CLEANING AND DECONTAMINATION

1. Spills of potentially infectious material should be cleaned up immediately with absorbent paper tissue and the contaminated area should be decontaminated with disinfectants such as 0.5% freshly prepared sodium hypochlorite [10 times dilution of 5% sodium hypochlorite (household bleach)] before continuing work.
2. Sodium hypochlorite should not be used on an acid-containing spill unless the spill- area is wiped dry first. Materials used to clean spills, including gloves should be disposed off as potentially bio-hazardous waste e.g. in a bio-hazard waste container.

14. TEST PROCEDURE

(Please also refer the **Truelab®** Real Time micro PCR Analyzer user manual)

1. Switch on the **Truelab®** Analyzer.
2. Select User and enter password.
3. For **Truelab® Uno Dx**, select the test profile for "Malaria Pf" to be run from the Profiles Screen on the Analyzer screen. For **Truelab® Duo/Quattro**, select the Bay (Idle1/2) for **Duo** and (Idle1/2/3/4) for **Quattro** from the Status Screen to view the Profiles Screen. Select the test profile for "Malaria Pf" to be run from the Profiles Screen on the Analyzer screen.
4. Enter the patient details as prompted in the **Truelab®** Analyzer screen.
5. Press Start Reaction.
6. For **Truelab® Uno Dx**, Press the eject button to open the chip tray. For **Truelab®**

Duo/Quattro, the chip tray opens automatically on tapping the "Start Reaction" button.

7. Open a pouch of **Truenat® Malaria Pf** and retrieve the micro PCR chip, microtube and DNase & RNase free pipette tip.
8. Place the **Truenat® Malaria Pf** chip on the chip tray without touching the white reaction well. The reaction well should be facing up and away from the Analyzer. Gently press the chip to ensure that it has seated in the chip tray properly.
9. Place the microtube containing freeze dried PCR reagents in the microtube stand provided along with the **Truelab®** Real Time micro PCR workstation **after ensuring that white pellet of dried PCR reagents remains at the bottom of the microtube**. Remove the microtube cap and dispose it off as per the section on "Disposal and Destruction" (Section 17). Using the filter barrier tip provided in the pouch, pipette out six (6) µL of the purified DNA from the Elute Collection Tube into the microtube. Allow it to stand for 30-60 seconds to get a clear solution. **△ Do not mix it by tapping, shaking or by reverse pipetting**. Using the same filter barrier tip, pipette out six (6) µL of this clear solution and dispense into the centre of the white reaction well of the **Truenat® Malaria Pf** chip. Take care not to scratch the internal well surface and not to spill elute on the outside of the well. Dispose off the microtip as per the section on "Disposal and Destruction" (Section 17).
10. For **Truelab® Uno Dx**, slide the chip tray containing the **Truenat® Malaria Pf** chip-based Real Time PCR test loaded with the sample into the **Truelab®** Analyzer. Press Done on the "Please Load Sample" Alert message. For **Truelab® Duo/Quattro**, select "YES" at the Please load Sample prompt. Chip tray will close automatically and the reaction will start.
11. Read the result from the screen.
12. After the reaction is completed, for **Truelab® Uno Dx**, push the Eject button to eject the chip tray. For **Truelab® Duo/Quattro**, tap the "Open/Close Tray" button to eject the chip tray.
13. Take out the **Truenat® Malaria Pf** micro PCR chip at end of the test and dispose it off as per the section on "Disposal and Destruction" (Section 17).
14. Turn on **Truelab®** micro PCR printer and select print on the screen for printing out hard copy of the results. Test results are automatically stored and can be retrieved any time later. (Refer to **Truelab®** Analyzer manual).
15. Switch off the **Truelab®** Analyzer.

15. RESULTS & INTERPRETATIONS

Two amplification curves are displayed on the **Truelab®** Real Time micro PCR Analyzer screen to indicate the progress of the test. Either or both the target and the internal positive control (IPC)* curves will take a steep, exponential path when the fluorescence crosses the threshold value in case of positive samples. The Ct will depend on the number of parasite genomes in the sample. The target curve will remain horizontal throughout the test duration and the IPC curve will take an exponential path in case of negative samples. In case the IPC curve remains horizontal in a negative sample, the test is considered as Invalid. At the end of the test run, the results screen will display "DETECTED" for Positive result or "NOT DETECTED" for Negative result. The result screen would also display the Ct value and the parasite load in copies/mL for positive specimen. The result screen also displays the validity of the test run as "VALID" or "INVALID". Invalid samples have to be repeated with fresh specimen from the sample preparation stage. *While IPC will co-amplify in most positive cases also, in some specimen having a high target load, the IPC may not amplify, however the test run is still considered valid.

16. QUALITY CONTROL PROCEDURES

To ensure that the **Truelab®** Real Time micro PCR Analyzer is working accurately, run positive and negative controls from time to time. The **Truenat®** Positive Control kit- Panel IV (REF 801040008) containing Positive Control and Negative Control must be ordered separately. It is advisable to run controls under the following circumstances: • Whenever a new shipment of test kits is received. • When opening a new test kit lot. If the temperature of the storage area falls outside of 2-30°C. • By each new user prior to performing testing on clinical specimen.

17. DISPOSAL AND DESTRUCTION

1. Submerge the used content such as **Truenat® Malaria Pf** chip, microtube, microtube cap, transfer pipette, pipette tips, lysis buffer tube etc. in freshly prepared 0.5% sodium hypochlorite solution for 30 minutes before disposal as per the standard medical waste disposal guidelines.
2. Disinfect the solutions and/or solid waste containing biological samples before discarding them according to local regulations.
3. Samples and reagents of human and animal origin as well as contaminated materials, disposables, neutralized acids and other waste materials must be discarded according to local regulations after decontamination by immersion in a freshly prepared 0.5% of sodium hypochlorite for 30 minutes (1 volume of 5% sodium hypochlorite for 10 volumes of water).
4. Do not autoclave materials or solutions containing sodium hypochlorite.
5. Chemicals should be handled in accordance with Good Laboratory Practice and disposed off according to the local regulations.

18. SPECIFIC PERFORMANCE CHARACTERISTICS


Analytical Exclusivity (Primer specificity): The following microorganisms were

evaluated *in silico* from the NCBI database using the NCBI nucleotide blast and primer blast tools to determine potential cross-reactivity in the **Truenat® Malaria Pf** assay. Results obtained showed no cross reactivity of the **Truenat® Malaria Pf** assay with the listed organisms.

Bacteria	Virus
<i>Acinetobacter anitratus</i>	Human Papilloma virus
<i>Candida albicans</i>	Cytomegalovirus
<i>Gardnerella vaginalis</i>	Hepatitis B virus
<i>Enterobacter cloacae</i>	Epstein-Barr virus
<i>Salmonella enterica</i>	Simian virus
<i>Staphylococcus aureus</i>	Human Immunodeficiency virus
<i>Neisseria gonorrhoeae</i>	Hepatitis C virus
<i>Escherichia coli</i>	Herpes Simplex virus
<i>Streptococcus mutans</i>	Adenovirus
<i>Enterococcus faecalis</i>	
<i>Trichomonas vaginalis</i>	


Linearity:

Serial dilutions of *Plasmodium falciparum* plasmid DNA (from 6.1E+07copies/mL to 6.1E +03copies/mL) were made and nucleic acids were extracted on **Trueprep® AUTO** Universal Cartridge Based Sample Prep Device for each dilution followed by PCR on **Truelab®** Real Time micro PCR analyzer. The assay is found to be linear over 5 orders of magnitude (from 6.1E+07 copies/mL to 6.1E +03 copies/mL) for *Plasmodium falciparum* DNA as depicted in the given graph.

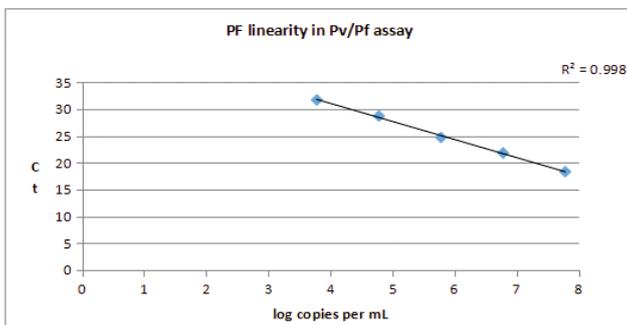

Limit of detection (LoD):

The LoD was determined by testing dilutions of *Plasmodium falciparum* plasmid DNA. Probit analysis of the data was used to determine the concentration of the DNA with 95% probability of detection. The LoD was found to be 1866 copies/mL for *Plasmodium falciparum* plasmid DNA.

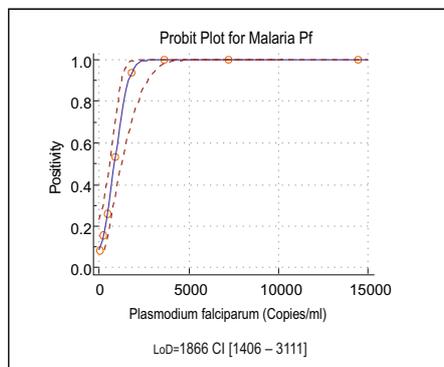

Robustness:

To determine whether the **Truenat® Malaria Pf** chip-based Real Time PCR test showed any signs of carryover of PCR products between runs, alternating runs of positive samples and negatives samples were performed. 10 positive samples and 10 negative samples were used for the study. The **Truenat® Malaria Pf** test did not exhibit detectable carryover contamination between positive to negative sample runs.

Reproducibility:

The purpose of this study is to compare the functional performance of the **Truenat® Malaria Pf** assay using three different titres of samples on **Truelab® Uno Dx** Real Time micro PCR analyzer. High, Medium and low titre samples were extracted on **Trueprep® AUTO** Universal Cartridge Based Sample Prep Device and tested among three different users (Inter user), on three different devices (Inter device) and on 5 consecutive days (Inter day) to check the variability. Mean %CV values for all titres has been calculated for Malaria Pf as Inter User (1.78), Inter day (2.30) and Inter Device (2.08) which were in the accepted range of ≤15% CV for **Truenat® Malaria Pf** assay.

Precision:

Precision was tested by performing **Truenat® Malaria Pf** assay with extracted DNA of

High (6.1E+05 copies/mL), Medium (6.1E+04 copies/mL) and Low (6.1E+03 copies/mL) titres for Malaria Pf for five consecutive days. Every day PCR for each titre DNA was run in triplicates. The %CV values obtained for High titre (1.50), Medium titre (2.00) and low titre (4.62) for Malaria Pf were within the accepted range of ≤15% CV for **Truenat® Malaria Pf** assay.

19. REFERENCES

- Rich, S. M. et al (2009) "The origin of malignant malaria". Proceedings of the National Academy of Sciences 106(35): 14902-14907.
- Perlmann, P. et. al. (2000). "Malaria blood-stage infection and its control by the immune system". Folia biologica 46 (6): 210-218.
- Marchand RP, et. al. (2011). Co-infections of *Plasmodium knowlesi*, *P. falciparum*, and *P. vivax* among Humans and Anopheles Mosquitoes, Southern Vietnam. *Emerg Infect Dis*. Jul 2011; 17(7):1232-1239.
- Moody A. (2002) Rapid diagnostic tests for malaria parasites. *Clin Microbiol Rev* 2002; 15:66-78.
- Andrade et. al. (2010). Towards a precise test for malaria diagnosis in the Brazilian Amazon: comparison among field microscopy, a rapid diagnostic test, nested PCR, and a computational expert system based on artificial neural networks. *Malaria Journal* 2010;9: 117.
- Khairnar K, et al. (2009) Multiplex real-time quantitative PCR, microscopy and rapid diagnostic immuno-chromatographic tests for the detection of *Plasmodium spp*: performance, limit of detection analysis and quality assurance. *Malar J* 2009, 8:284.
- Shokoples S.E. et al. (2009). Multiplexed real-time PCR assay for discrimination of *Plasmodium* species with improved sensitivity for mixed infections. *J Clin Microbiol* 2009, 47:975-980.
- WHO-FIND-CDC Malaria RDT Product Testing Methods Manual (Version 1)-05/2008.
- Adams JH et al. (1992) A family of erythrocyte binding proteins of malaria parasites. *Proc Natl Acad Sci USA* 89, 7085-7089.
- Pascal Michon et al. (2002). Evolutionary Relationships of Conserved Cysteine-Rich Motifs in Adhesive Molecules of Malaria Parasites. *Mol Biol Evol* 2002, 19(7):1128-1142.

SYMBOL KEYS

 Consult instructions for use	IVD In vitro Diagnostic Medical Device. Not for medicinal use.	 Temperature Limitation	REF Catalogue Number	 For single use only	 This Side Up	 Manufacturer
 Date of Manufacture	 Date of Expiry	LOT Batch Number / Lot Number	 Caution	 Contains sufficient for <n> tests	EC REP Authorised Representative in the European Community	



Molbio Diagnostics Private Limited

Registered Office & Manufacturing Unit - I:

Plot No. L-46, Phase II D, Verna Industrial Estate, Verna, Goa - 403 722, INDIA

Manufacturing Unit - II:

Plot No. L-42, Phase II B, Verna Industrial Estate, Verna, Goa - 403 722, INDIA

www.molbiodiagnostics.com Email: sales@molbiodiagnostics.com

EC REP Qarad EC-REP BV, Pas 257, 2440 Geel, Belgium